

This Page Is Inserted by IFW Operations  
and is not a part of the Official Record

## **BEST AVAILABLE IMAGES**

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS

**IMAGES ARE BEST AVAILABLE COPY.**

**As rescanning documents *will not* correct images,  
please do not report the images to the  
Image Problem Mailbox.**

# 中華民國專利公報 [19] [12]

[11]公告編號：386030

[44]中華民國 89年(2000) 04月01日  
發明

全 5 頁

[51] Int.Cl. 06: A61F13/15

[54]名稱：單片包裝衛生擦拭物

[21]申請案號：087119339

[22]申請日期：中華民國 88年(1999) 06月04日

[30]優先權：[31]08/975,792

[32]1997/11/21 [33]美國

[72]發明人：

湯瑪斯瓦德奧斯伯三世

美國

[71]申請人：

寶鹼公司

美國

[74]代理人：陳長文 先生

1

2

[57]申請專利範圍：

- 1.一種用於一吸收性陰唇間裝置之一單片包裝件，其中該吸收性陰唇間裝置將至少部分插入用者陰唇間空間內，該單片包裝件包括：  
一裹件，用以包裝該吸收性陰唇間裝置，該裹件包含一撓性頁，其至少部分沿該吸收性陰唇間裝置周圍纏繞，該撓性頁具有一與該吸收性陰唇間裝置相鄰之吸收內表面，當該裹件開啟時，其在該吸收性陰唇間裝置插入該陰唇間空間內時提供用者一衛生擦拭裝置，以擦拭陰唇。  
2.如申請專利範圍第1項之單片包裝件，其中該裹件包含至少係由下列各物中選出之一者：薄紙；膠原膜；熱塑膜；不織布材料；熱塑膜與薄紙之疊層；膠原膜與薄紙之疊層；熱塑膜與不織布材料之疊層；膠原膜與熱塑膜之疊層。  
3.如申請專利範圍第1項之單片包裝件，其中該裹件具有一外表面，且該外表面係為液體不可穿透。  
4.如申請專利範圍第1項之單片包裝件，其足可沖棄，在沖棄性測試時，至少70%次數中，以兩次或以下沖棄完全清除該桶。  
5.如申請專利範圍第1項之單片包裝件，其足可沖棄，在沖棄性測試時，至少95%次數中，以一次沖棄完全清除該桶。  
6.如申請專利範圍第1項之單片包裝件，其中在散水實驗中，測量該裹件散成至少兩片斷所需時間，小於約2小時。  
7.如申請專利範圍第1項之單片包裝件，其中該裹件造成小於80%之排水阻塞。  
8.一種個別包裝吸收性陰唇間裝置，其中該吸收性陰唇間裝置包含：  
一中央吸收部，其包含一縱尺寸、一寬度、一高度，其中該縱尺寸大於該高度  
一上部、及一下部，該上部在插入該陰
- 10.
- 15.
- 20.

唇間空間內期間面對該用者的前腔底面，並在插入該處時引導該下部，該上部具有一縱軸，該下部與該上部相對，且當該吸收裝置插入該陰唇間裝置內時，該下部朝向離開該用者前腔底面方向；及

一單片包裝件，其用於該吸收性陰唇間裝置，其包含一撓性頁，其沿該吸收性陰唇間裝置相對於該下部縱軸摺疊，形成一縱摺、縱緣、及橫側緣，其中該縱緣及該橫側緣密封形成該單片包裝件，當該單片包裝件開啟時，其在將該吸收性陰唇間裝置插入該陰唇間空間內時提供用者一衛生擦拭裝置以擦拭陰唇。

圖式簡單說明：

第一圖為一吸收性陰唇間裝置其一實施例之透視圖。

第二圖為第一圖所示吸收裝置之一端視圖。

第三圖為一吸收性陰唇間裝置其另一實施例之一透視圖。

第四圖為本發明之單片包裝件其一較佳實施例之一側視圖。

5. 第五圖係為圍繞並包括用者身體大陰唇及小陰唇之一透視圖，其中顯示本發明如何用來保護用者手指。


第六圖為本發明之另一較佳實施例其一側視圖，其中顯示開啟該包裝件之一前簾片。

第七圖為本發明之另一較佳實施例其一側視圖，其中顯示開啟該包裝件之一側簾片。

第八圖為本發明之一部分開啟包裝件其一透視圖。


第九圖為適合該沖棄性測試之裝置之一俯視圖。

第十圖為第九圖中該裝置其一部分管件之一剖視圖。

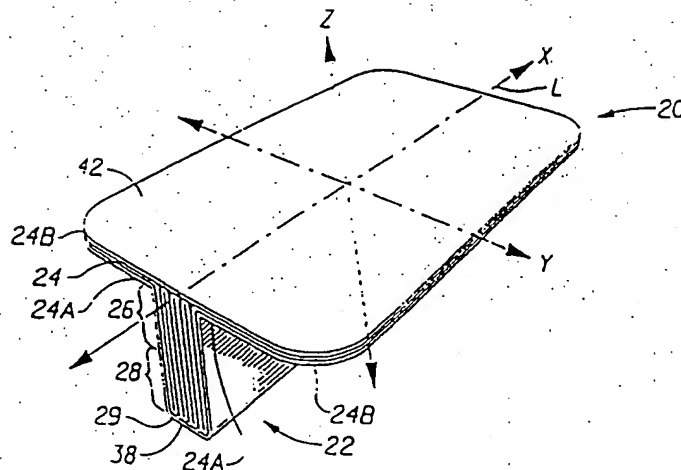


第一圖


(3)

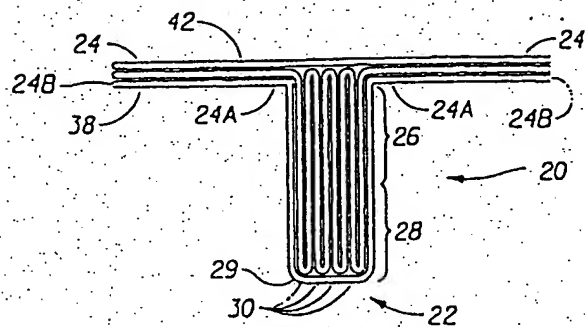


第二圖

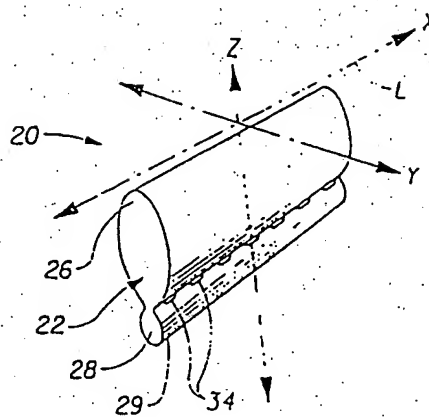

第三圖

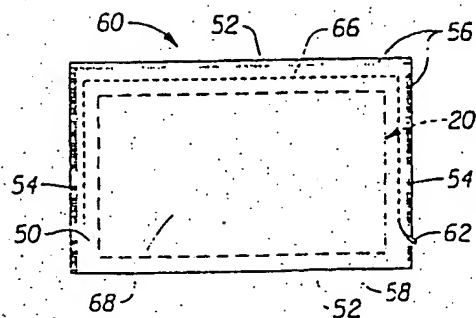



第四圖

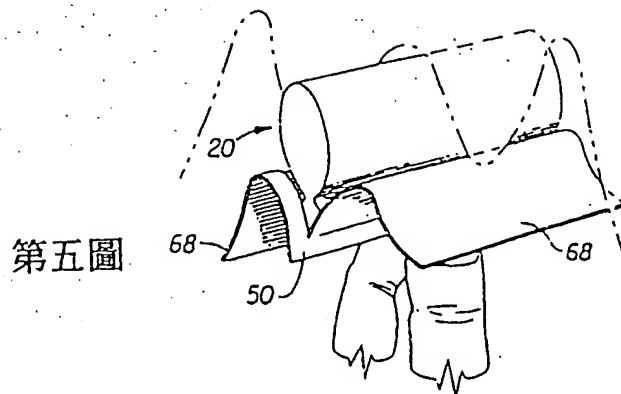

第五圖



(4)

第六圖

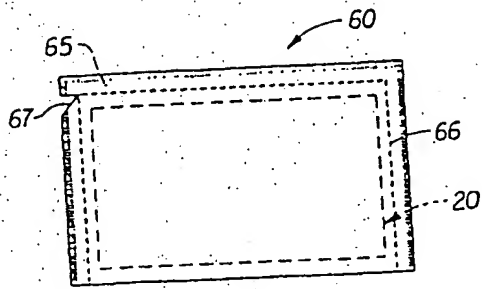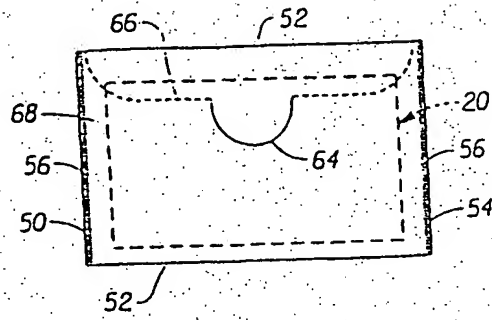


第七圖

第八圖

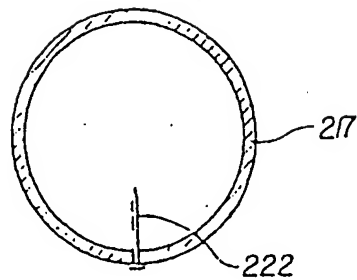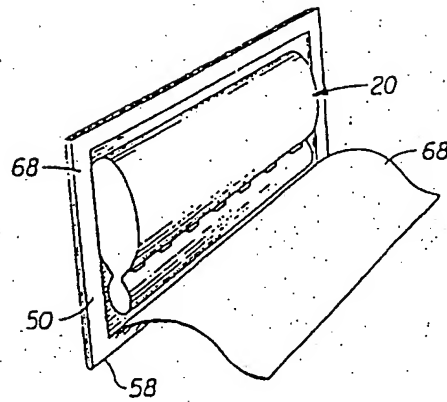

第十圖

(5)

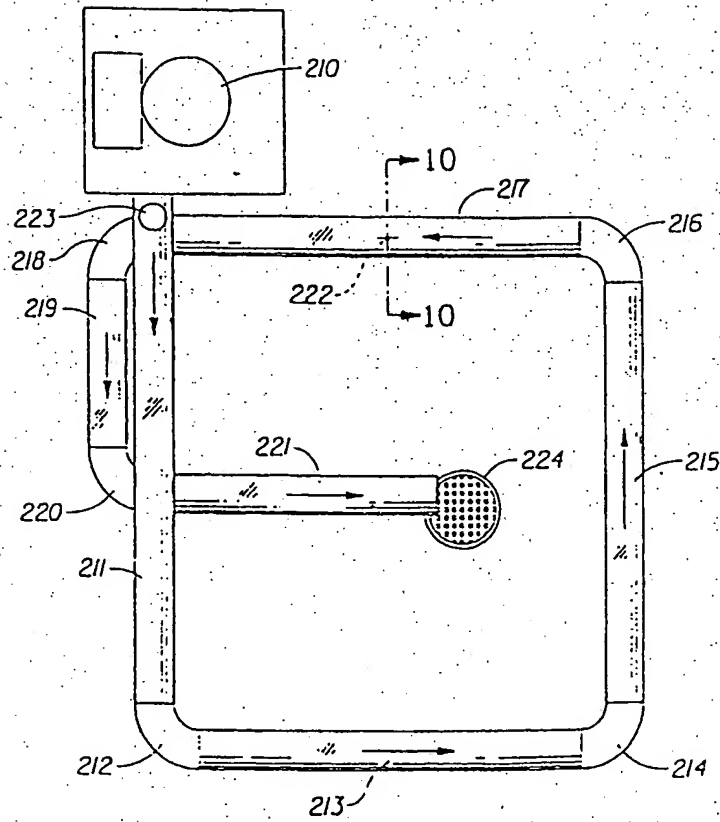

第九圖

ABSTRACT OF THE DISCLOSURE

Individual packages to assist the hygienic insertion of an absorbent device into the interlabial space of a female user are disclosed. The individual package comprises a wrapper for packaging the absorbent device. The wrapper comprises a flexible sheet which is wrapped around the absorbent device. The flexible sheet has an absorbent inside surface adjacent to the absorbent interlabial device, which when the wrapper is opened, provides the user with a sanitary wiping device to wipe the labia while inserting said absorbent interlabial device into the interlabial space. In one embodiment, the wrapper is folded about the absorbent device relative to the longitudinal axis of the lower portion of the absorbent interlabial device forming a longitudinal fold, an opposing open end, and transverse side edges. The opposing open end and transverse side edges are sealed to form the individual package.

## INDIVIDUAL PACKAGING FOR HYGIENIC WIPING

FIELD OF THE INVENTION

5 This invention relates to individual packages for absorbent devices that are worn interlabially by female wearers for catamenial purposes, incontinence protection, or both. More particularly, the present invention relates to individual packages to provide the user with a sanitary wiping device to wipe the labia while inserting the absorbent interlabial device into the interlabial space.

BACKGROUND OF THE INVENTION

10 All manner and variety of absorbent articles configured for the absorption of body fluids such as menses, urine and feces are, of course, well known. With respect to feminine protection devices, the art has offered two basic types; sanitary napkins have been developed for external wear about the pudendal region while tampons have been developed for internal wear within the vaginal cavity for interruption of menstrual flow therefrom. Such tampon devices are disclosed in U.S. Patent No. 4,412,833, entitled "Tampon Applicator," issued to Weigner, et al. on November 1, 1983, and U.S. Patent No. 4,413,986, entitled "Tampon Assembly With Means For Sterile Insertion", issued to Jacobs on November 8, 1983.

20 Hybrid devices that attempt to merge the structural features of the sanitary napkins and the tampons into a single device have also been proposed. Such hybrid devices are disclosed in U.S. Patent No. 2,092,346, entitled "Catamenial Pad," issued to Arone on September 7, 1937, and U.S. Patent No. 3,905,372, entitled "Feminine Hygiene Protective Shield," issued to Denkinger on September 16, 1975. Other less intrusive hybrid devices are known as labial or interlabial sanitary napkins and are characterized by having a portion which at least partially resides within the wearer's vestibule and a portion which at least partially resides external of the wearer's vestibule. Such devices are disclosed in U.S. Patent No. 2,662,527, entitled "Sanitary Pad," issued to Jacks on December 15, 1953, and U.S. Patent No. 4,631,062, entitled "Labial Sanitary Pad," issued to Lassen, et al. on December 23, 1986.



Interlabial pads have the potential to provide even greater freedom from inconvenience because of their small size and reduced risk of leakage. Numerous attempts have been made in the past to produce an interlabial pad which would combine the best features of tampons and sanitary napkins while avoiding at least some of the disadvantages associated with each of these types of devices. Examples of such devices are described in U.S. Patent 2,917,049 issued to Delaney on December 15, 1959, U.S. Patent 3,420,235 issued to Harmon on January 7, 1969, and U.S. Patent 4,595,392 issued to Johnson, et al. on June 17, 1986. A commercially available interlabial device is FRESH 'N' FIT® PADETTE® interlabial product that is marketed by Athena Medical Corp. of Portland, OR and described in U.S. Patents 3,983,873 and 4,175,561 issued to Hirschman on October 5, 1976 and November 27, 1979, respectively.

If the consumer needs only one interlabial pad for later use, the consumer must take precautions to protect the interlabial pad from soiling or contamination from the time it is removed from the box or bag until the article is used. This is a particular concern with respect to maintaining a sanitary environment during insertion and removal. That is, a need exists to hygienically store an individual interlabial pad while being transported to prevent transferring unsanitary particles to the interlabial space. Additional needs also exist for providing a hygienic and clean environment in and around the labial space.

The packaging for the commercially available FRESH 'N' FIT® PADETTE® interlabial product is made from a coated paper sheet that is wrapped around the product and sealed on the transverse ends and along the longitudinal edges. The transverse ends and longitudinal edges of the product are sealed with an adhesive and are then crimped together. Another example of packaging for an interlabial pad is shown in U.S. Patent 4,743,245 entitled "Labial Sanitary Pad" that issued to F. O. Lassen, et al. on May 10, 1988. However, there are drawbacks to these packages.

One important drawback is that these wrappers do not provide a means for users of interlabial products to preserve hygiene when inserting an interlabial device into the folds of the skin. The lack of hygiene in restrooms, the need to touch the doors of nonhygienic restrooms, and the necessity to touch themselves while inserting the device may result in the possibility of infection. In addition, when inserting the device during menstruation, it is desirable to keep the user's hands free

from soiling. Therefore, the consumer needs an individual package that will protect the user's hand, fingers and the hygienic nature of the product.

Other packages for sanitary articles are described in U.S. Patent 3,062,371 entitled "Internally Sterile Composite Package" that issued to D. Patience on November 6, 1962 and U.S. Patent 3,698,549 entitled "Packages for Small Articles" that issued to J. A. Glassman on October 17, 1972. The Patience patent describes a package that is opened by folding back a panel from the package and removing its content by using sterile forceps. The Glassman patent describes a package that has internal pockets for holding flat articles such as gauze dressings or surgical sponges. The package is opened and exposes separate pockets for removal of individual articles.

Although the packages described in the Patience patent, the Glassman patent, the wrapper used with the PADETTE® product, and the wrapper described in the Lassen patent protect the enclosed article, the package or wrapper does not aid in the hygienic insertion and placement of the product or provide a barrier to prevent the wearer's hand from touching the product or the wearer's body.

Packages for tampons are described in U.S. Patent 3,135,262 entitled "Tampon" that, issued to W. Kobler, et al. on June 2, 1964 and U.S. Patent 5,180,059 entitled "Package of a Sanitary Tampon" that issued to S. Shimatani and K. Shimatani on January 19, 1993. The Kobler patent describes a wrapper that when unwrapped, forms what Kobler describes as an umbrella to cover the user's hands. Because of the shape of the tampon (the height of the tampon is considerably greater than the tampon's longitudinal dimension), the wrapper must be considerably longer than the tampon to encircle the user's hand when opened. When the wrapper is opened, the material that forms the shield is large and would be an impediment to proper placement. Additionally, the wrapper in the Kobler patent does not completely seal all parts of the product inside the package creating the potential for contamination. Specifically, the tear cord used to break the band that holds the wrapper onto the tampon must be touched by the user. The same cord, when the tampon is in use, then resides in the vaginal region that is sensitive to contamination.

The Shimatani patent describes a package that comprises packing sheets superimposed on another to enclose the tampon to create a shield when inserting the tampon. This patent fails to provide a sterile environment because it, too, does not seal all parts of the product inside the package that should be protected from

contamination or prevent the user from touching parts that should maintain sterility. Additionally, the stiffness of the Shimatani package would not provide the user comfort when inserting the article.

5 The packages for the Kobler and Shimatani patents are tall and circular in shape. The Kobler and Shimatani packages may be suitable in packaging articles that have a height greater than its longitudinal dimension, however, with smaller articles such as an interlabial product where its longitudinal dimension is greater than the article's height, such a wrapper would not be feasible. The package of the present invention is flat in comparison and uses side panels to provide the user hygienic,  
10 comfortable insertion and placement of the interlabial device. Also, the package of the present invention differs from the Kobler and Shimatani packages because they are not flushable or biodegradable.

Therefore, it is an object of the present invention to provide a hygienic individual package for an interlabial device.

15 It is another object of the present invention to provide an individual package for an interlabial device that facilitates hygienic insertion of the device.

It is another object of the present invention to provide a hygienic individual package for an interlabial device that is flushable and biodegradable.

20 It is yet another object of the present invention to provide a sanitary wiping device to wipe the labia while inserting the absorbent interlabial device into the interlabial space.

These and other objects of the present invention will become more readily apparent when considered in reference to the following description and when taken in conjunction with the accompanying drawings.

25

### SUMMARY OF THE INVENTION

This invention relates to individual packages for absorbent devices that are worn interlabially by female wearers for catamenial purposes, incontinence protection, or both. More particularly, the present invention relates to individual  
30 packages that provide the user with a sanitary wiping device to wipe the labia while inserting the absorbent interlabial device into the interlabial space.

The individual package comprises a wrapper for packaging the absorbent interlabial device. The absorbent interlabial device has a width, a height and a longitudinal dimension that is greater than the height. The absorbent interlabial device is to be inserted at least partially within a user's interlabial space with the longitudinal dimension running lengthwise in the interlabial space. The wrapper comprises a flexible sheet that is wrapped around the absorbent interlabial device. The absorbent device has a longitudinal axis, an upper portion and a lower portion. The wrapper is preferably folded about the absorbent device relative to the longitudinal axis of the absorbent device forming a longitudinal fold, an opposing open end, and transverse side edges. In this preferred embodiment, the opposing open end and transverse side edges are sealed to form the individual package.

The flexible sheet has an absorbent inside surface adjacent to the absorbent interlabial device, which when the wrapper is opened, provides the user with a sanitary wiping device to wipe the labia while inserting said absorbent interlabial device into the interlabial space. The wrapper also protects the absorbent interlabial device during storage and transportation by shielding the interlabial device from contamination.

20

#### BRIEF DESCRIPTION OF THE DRAWINGS

While the specification concludes with claims particularly pointing out and distinctly claiming the subject matter that is regarded as forming the present invention, it is believed that the invention will be better understood from the following description taken in conjunction with the accompanying drawings, in which:

25

FIG. 1 is a perspective view of one embodiment of an absorbent interlabial device.

FIG. 2 is an end view of the absorbent device shown in FIG. 1.

FIG. 3 is a perspective view of another embodiment of an absorbent interlabial device.

30

FIG. 4 is a side view of a preferred embodiment of the individual package of the present invention.

FIG. 5 is a perspective view of a wearer's body surrounding and including the wearer's labia majora and labia minora showing how the present invention is used to protect the user's fingers.

FIG. 6 is a side view of an alternative preferred embodiment of the present invention showing a front tab for opening the package.

FIG. 7 is a side view of an alternative preferred embodiment of the present invention showing a side tab for opening the package.

FIG. 8 is a perspective view of a partially opened package of the present invention.

FIG. 9 is a top plan view of the apparatus suitable for the Flushability Test.

FIG. 10 is a cross sectional view of a portion of piping of the apparatus in FIG. 9.

#### DETAILED DESCRIPTION OF THE INVENTION

The present invention is directed to an individual package for an absorbent interlabial device. FIG. 1 shows one preferred embodiment of the absorbent interlabial device 20. The interlabial device, however, can be in many other forms, and is not limited to a structure having the particular configuration shown in the drawings.

As used herein, the term "absorbent interlabial device" refers to a structure that has at least some absorbent components, and is specifically configured to reside at least partially within the interlabial space of a female wearer during use. Preferably, more than half of the entire absorbent interlabial device 20 resides within such interlabial space, more preferably substantially the entire absorbent interlabial device 20 resides within such interlabial space, and most preferably the entire absorbent interlabial device 20 resides within such interlabial space of a female wearer during use.

As used herein, the term "interlabial space" refers to that space in the pudendal region of the female anatomy that is located between the inside surfaces of the labia majora extending into the vestibule. Located within this interlabial space are the labia minor, the vestibule and the principal urogenital members including the clitoris, the orifice of the urethra, and the orifice of the vagina. Standard medical authorities teach that the vestibule refers to the space bounded laterally by the inside surfaces of the labia minora and extending interiorly to the floor between the clitoris and the orifice of the vagina. Therefore, it will be recognized that the interlabial space as defined above may refer to the space between the inside surfaces of the labia majora, including the space between the inside surfaces of the labia minora also known as the vestibule. The interlabial space for purposes of the present description does not extend substantially beyond the orifice of the vagina into the vaginal interior.

The term "labia" as used herein refers generally to both the labia majora and labia minora. The labia terminate anteriorly and posteriorly at the anterior commissure and the posterior commissure, respectively. It will be recognized by those skilled in the art that there is a wide range of variation among women with respect to the relative size and shape of labia majora and labial minora. For purposes of the present description, however, such differences need not be specifically addressed. It will be recognized that the disposition of the absorbent interlabial device into the interlabial space of a wearer as defined above will require placement between the inside surfaces of the labia majora without regard to the precise location of the boundary between the labia majora and the labia minora for a particular wearer. For a more detailed description of this portion of the female anatomy, attention is directed to *Gray's Anatomy*, Running Press 1901 Ed. (1974), at 1025-1027.

The absorbent interlabial device 20 shown in FIG. 1 has a longitudinal centerline L that runs along the "x" axis shown in FIG. 1. The term "longitudinal," as used herein, refers to a line, dimension, axis or direction in the plane of the interlabial device 20 that is generally aligned with (e.g., approximately parallel to) a vertical plane that bisects a standing wearer into left and right body halves and extends between the front and rear of the wearer's body when the interlabial device 20 is worn. The terms "transverse" and "lateral" as used herein, are interchangeable, and refer to a line axis or direction that is generally perpendicular to the longitudinal direction (that is, in a direction outward from this vertical plane toward the wearer's thighs). The lateral direction is shown in FIG. 1 as the "y" axis. The "z" direction,

shown in FIG. 1, is a direction parallel to the vertical plane described above. The term "upper" refers to an orientation in the z-direction toward the wearer's head. "Lower" or downwardly is toward the wearer's feet.

In the embodiment shown in FIG. 1, the interlabial device 20 comprises a central absorbent portion (or "main absorbent") 22, and optionally, a pair of flexible extensions 24 joined to the central absorbent portion 22. The central absorbent portion 22 should be at least partially absorbent. The central absorbent portion 22 may comprise non-absorbent portions, such as a liquid impervious barrier to prevent absorbed exudates from leaking out of the central absorbent portion 22. The central absorbent portion 22 comprises an upper portion 26 and a lower portion 28 that is opposed to the upper portion. As shown in FIGS. 1 and 2, when the central absorbent portion 22 is of a uniform transverse dimension (i.e., there is no abrupt change in transverse dimension defining the juncture between the upper portion and lower portion) the division between the upper portion 26 and lower portion 28 is considered to be at a height equal to about one-half of the total height of the central absorbent portion 22. The flexible extensions 24 are joined to the upper portion 26 of the central absorbent portion. In use, the upper portion 26 is positioned furthest inward into the wearer's interlabial space. The lower portion 28 has a base (or "bottom edge" or "lower edge") 29.

The interlabial device 20 should be of a suitable size and shape that allows at least a portion thereof to fit comfortably within the wearer's interlabial space and to cover the wearer's vaginal orifice, and preferably also the wearer's urethra. The interlabial device 20 at least partially blocks, and more preferably completely blocks and intercepts the flow of menses, urine, and other bodily exudates from the wearer's vaginal orifice and urethra.

The size of the interlabial device 20 is also important to the comfort associated with wearing the device. In the embodiment shown in FIGS. 1, 2 and 3, the width of the central absorbent portion 22 of the interlabial device 20 as measured in the transverse direction (y-direction) is preferably between about 2 mm and less than or equal to about 12 mm, more preferably between about 3 mm and about 8 mm. In a preferred embodiment, the width of the central absorbent portion of the interlabial device 20 is about 4.5 mm. The central absorbent portion 22 of the interlabial device 20 has a length as measured along the longitudinal centerline, L, of between about 35 mm and about 120 mm. Preferably, the length of the interlabial device 20 is between about 45 mm and about 100 mm, and more preferably, is about

49 mm. The height (or "z"-direction dimension) of the central absorbent portion 22 is preferably between about 8 mm and about 35 mm, and more preferably is about 20 mm. Caliper measurements given herein were measured using an AMES gage with a 0.25 psi (gauge) load and a 0.96 inch diameter foot. Those skilled in the art will recognize that if a 0.96 inch diameter foot is not appropriate for a particular sample size, the foot size may be varied while the load on the gauge is accordingly varied to maintain a confining pressure of 0.25 psi (gauge).

The interlabial device 20 is preferably provided with sufficient absorbency to absorb and retain the exudates discharged from the wearer's body. The capacity of the product, however, is dependent at least partially upon the physical volume of the absorbent interlabial device 20, particularly the central absorbent portion 22 thereof. The central absorbent portion 22 preferably has a capacity of at least about 1 g of 0.9% by weight saline solution, and may have a capacity of up to about 30 g by using absorbent gels or foams that expand when wet. Capacities may typically range from about 2 to about 10 grams, for saline. Those skilled in the art will recognize that the capacity for absorption of body exudates such as menses will typically be smaller than the capacities given above for absorption of saline. Since the interlabial space can expand, larger volumes can be stored in the interlabial space, if the fluid is stored as a gel, which adjusts to the body pressures. Additionally, if the absorbent interlabial device 20 does not reside completely within the wearer's interlabial space, some of the absorbed exudates may be stored externally to the wearer's interlabial space.

The central absorbent portion 22 of the interlabial device 20 may comprise any suitable type of absorbent structure that is capable of absorbing and/or retaining liquids (e.g. menses and/or urine). The central absorbent portion 22 may be manufactured in a wide variety of shapes. Non-limiting examples include ovoid, trapezoidal, rectangular, triangular, cylindrical, hemispherical or any combination of the above. The central absorbent portion 22 may, likewise, be manufactured from a wide variety of liquid-absorbent materials commonly used in absorbent articles such as comminuted wood pulp that is generally referred to as airfelt. Examples of other suitable absorbent materials include cotton; creped cellulose wadding; meltblown polymers including coform; chemically stiffened, modified or cross-linked cellulosic fibers; synthetic fibers such as crimped polyester fibers; peat moss; tissue including tissue wraps and tissue laminates; absorbent foams; absorbent sponges; superabsorbent polymers; absorbent gelling materials; or any equivalent material or combinations of materials, or mixtures of these. Preferred absorbent



materials comprise folded tissues, woven materials, nonwoven webs, needle punched rayon, and thin layers of foam. The central absorbent portion 22 may comprise a single material or a combination of materials, such as a wrapping layer surrounding a central wadding comprised of a different absorbent material.

5 In the embodiment shown in FIGS. 1 and 2, the central absorbent portion 22 of the absorbent interlabial device 20 comprises a pleated structure. As shown in FIGS. 1 and 2, the central absorbent portion 22 comprises a folded tissue web. The folded tissue web preferably has a strength greater than that of standard non-wet strength toilet tissue. Preferably, the central absorbent portion 22 comprises a tissue  
10 having a temporary wet strength of greater than or equal to about 100 g. In a preferred embodiment, this wet strength will decay to about 50% or less of the original strength over about 30 minutes when measured under a wet burst strength test.

As shown in FIGS. 1 and 2, the tissue web comprising the central absorbent  
15 portion 22 is folded into a pleated structure comprising a plurality of pleats 30 that are arranged in a laterally side-by-side relationship. The tissue web can be folded so that it has any suitable number of pleats. Preferably, the tissue web is folded so that the overall caliper (i.e., the width) of the central absorbent portion 22 of this embodiment is between about 2 mm and less than or equal to about 8 mm.

20 The pleats in the folded tissue web are preferably connected or joined (or retained) in some suitable manner so that the pleated sections maintain their pleated configuration, and are not able to fully open. The pleats can be connected by a variety of means including the use of thread, adhesives, or heat sealing tissues which contain a thermoplastic material, such as, polyethylene. A preferred design uses  
25 stitching which joins all of the pleats in the central absorbent portion 22 together with cotton fiber. Preferably, the main absorbent structure 22 is provided with five stitch locations (four at the corners and one additional location approximately midway between the two lower corners).

The pleated structure of the central absorbent portion 22 provides several  
30 advantages. One advantage provided by the pleated structure is that exudates can penetrate into the pleats of the structure which present a larger and more effective absorbent surface for acquisition than a flat surface. This is particularly important when dealing with potentially viscous fluids and particulate material such as cellular debris and clots which can plug the surface of the structure presented to the body. A

second advantage of this design is that the caliper (or width) of the product can be easily and conveniently controlled by varying the number of pleats. Another advantage of the pleated structure is that the number, thickness, and tightness of the pleats control the stiffness of the structure.

5 The stiffness of the central absorbent portion 22 is important for product comfort. If the central absorbent portion 22 is too flexible, the device is not conveniently or easily placed between the folds of the labia, if it is too stiff, the device is uncomfortable and when the user is in a sitting position, the product can be forced forward against the clitoris causing discomfort. The central absorbent portion  
10 22 preferably has a stiffness approximately equal to that of the products described in U.S. Patents 4,995,150 and 4,095,542.

In the embodiment shown in FIG. 3, the central absorbent portion 22 is formed of a soft absorbent material such as rayon fibers or other suitable natural or synthetic fibers or sheeting. The central absorbent portion 22 shown in FIG. 3 is  
15 generally of an ovoid cross sectional shape. The central absorbent portion 22 of the embodiment shown in FIG. 3 comprises an upper portion 26 with a larger transverse sectional dimension relative to that of the lower portion 28. The upper portion 26 is preferably integral with the lower portion 28. In less preferred embodiments, however, the upper portion 26 and lower portion 28 may comprise separate elements  
20 joined together by any suitable means known in the art. In the embodiment shown in FIG. 3, the juncture of the upper portion 26 and lower portion 28 of the central absorbent portion 22 comprises a substantially abrupt change in the transverse dimension thereby forming a shoulder-like configuration at such juncture. In the embodiment shown in FIG. 3, the juncture of the upper portion 26 and lower portion  
25 28 of the central absorbent portion 22 is formed by stitching 34.

In a variation of the embodiment described above and shown in FIG. 3, the upper portion 26 may have a smaller transverse sectional dimension relative to the transverse sectional dimension of the lower portion 28, and the portions may have different absorbent capacities. In other embodiments, such as that shown in FIGS. 1  
30 and 2, the juncture between the upper portion 26 and the lower portion 28 can be indistinguishable.

The central absorbent portion 22 can be made by any suitable process. U.S. Patent 4,995,150 issued to Gerstenberger et al. on February 26, 1991 and U.S. Patent 4,095, 542 issued to Hirschman on June 20, 1978 describe methods for making

absorbent devices which are suitable for use as the central absorbent portion 22 of the absorbent interlabial device 20 shown in FIG. 3.

As shown in FIGS. 1 and 2, the absorbent interlabial device 20 preferably also comprises a pair of flexible extensions 24 which are joined to the upper portion 26 of the central absorbent portion 22 of the absorbent interlabial device 20. In the preferred embodiment shown in FIGS. 1 and 2, the flexible extensions 24 are generally rectangular in shape. Other shapes are also possible for the flexible extensions 24 such as semi-circular, trapezoidal, or triangular. The flexible extensions 24 preferably are from about 40 mm to about 160 mm in length, more preferably from about 45 mm to about 130 mm in length, and most preferably from about 50 mm to about 115 mm in length. While the flexible extensions 24 can have a length (measured in the x-direction) which is shorter than the central absorbent portion 22, preferably they have a length which is the same as or longer than the central absorbent portion 22 of the absorbent interlabial device 20. The width of each flexible extensions refers to the distance from the attachment of flexible extension 24 to the central absorbent portion 22 (or the proximal end 24A of the flexible extension 24) to the distal end (or free end) 24B of the flexible extension 24. The width of the flexible extensions 24 is preferably about equal to or greater than the height of the central absorbent portion as described above. The caliper of the flexible extensions is preferably less than or equal to about 3 mm, more preferably less than or equal to about 2 mm, and most preferably less than or equal to about 1 mm. Ideally, the caliper of the flexible extensions 24 and the central absorbent portion 22 are selected such that the caliper of the overall absorbent interlabial structure 20 is less than or equal to about 8 mm.

The flexible extensions 24 may be constructed of a tissue layer. A suitable tissue is an airlaid tissue available from Fort Howard Tissue Company of Green Bay, Wisconsin, and having a basis weight of 35 lbs./3000 sq. ft. Another suitable airlaid tissue is available from Merfin Hygienic Products, Ltd., of Delta, British Columbia, Canada, having a basis weight of 61 g/m<sup>2</sup> and having the designation grade number 176. Still another suitable material is an airlaid cotton batt such as that sold as cosmetic squares by Revco Stores, Inc. of Twinsburg, OH. The flexible extensions 24 may optionally be backed with a layer of material which is impervious or semi-pervious to body exudates such as polyethylene, polypropylene, or a polyvinylalcohol.

In the embodiment shown in FIGS. 1 and 2, the pair of flexible extensions 24 may comprise a single sheet of material extending to either side of the longitudinal centerline L of the central absorbent portion 22 of the absorbent interlabial device 20. Alternatively, the pair of flexible extensions 24 may comprise separate sheets of material independently joined to the upper portion 26 of the central absorbent portion 22. Preferably, the flexible extensions 24 are arranged symmetrically about the longitudinal centerline L of the central absorbent portion 22. The flexible extensions 24 are joined to the upper portion 26 of the central absorbent portion 22 of the absorbent interlabial device 20. Most preferably, the flexible extensions are joined to the top surface of the upper portion 26 of the central absorbent portion 22, or within about 5 mm of the top surface of the central absorbent portion 22.

The term "joined", as used herein, encompasses configurations in which an element is directly secured to another element by affixing the element directly to the other element; configurations in which the element is indirectly secured to the other element by affixing the element to intermediate member(s) which in turn are affixed to the other element; and configurations in which one element is integral with another element; i.e., one element is essentially part of the other element.

As shown in FIGS. 1 and 2, the flexible extensions 24 are attached to the upper portion 26 of the central absorbent portion 22. The flexible extensions 24 extend downwardly and outwardly from the central absorbent portion 22 to a free end 24B which is unattached to the central absorbent portion. The flexible extensions 24 may be biased slightly outward from the central absorbent portion 22 so as to tend to keep the extensions 24 in contact with the inner surfaces of the labia when the absorbent interlabial device 20 is in place. Additionally, the naturally moist surfaces of the labia will have a tendency to adhere to the material comprising the flexible extensions 24 further tending to keep them in contact with the inner surfaces of the labia. Preferably, the flexible extensions 24 should be capable of motion from a position where the free ends of the flexible extensions 24 lie adjacent to the central absorbent portion 22 to a position where the flexible extensions 24 extend directly out from the central absorbent portion 22 in the transverse direction.

The flexible extensions 24 may be joined to the upper portion 26 of the central absorbent portion 22 by any variety of means. For example, in the embodiment shown in FIGS. 3, flexible extensions 24 may be joined to the upper portion 26 using any suitable adhesive centered about the longitudinal centerline L of the central absorbent portion 22 (i.e., on opposite sides of the longitudinal

centerline L). The adhesive may extend continuously along the length of the central absorbent portion 22 or it may be applied in a "dotted" fashion at discrete intervals. Alternatively, the flexible extensions 24 may be joined to the upper portion 26 of the central absorbent portion 22 by stitching (such as with cotton or rayon thread), thermally bonding, fusion bonding, or any other suitable means known in the art for joining such materials.

The flexible extensions 24 should be of sufficient width and flexibility to allow the flexible extensions to cover the wearer's fingertips as the absorbent interlabial device 20 is inserted into the wearer's interlabial space. Additionally, the flexible extensions 24 should be capable of moving with the inner surfaces of the wearer's labia to maintain contact with the same. The flexible extensions 24 help keep the central absorbent portion 22 in place throughout a range of wearer motions such as squatting.

The flexible extensions 24 may be hydrophilic or hydrophobic. The flexible extensions 24 may be treated to make them less hydrophilic than the central absorbent portion 22. The hydrophilicity of a material is generally expressed in terms of its contact angle. Thus, the flexible extensions 24 may have an advancing contact angle greater than the advancing contact angle of the central absorbent portion 22, such that fluid is preferentially directed toward and absorbed by the central absorbent portion 22. The flexible extensions 24 may be either absorbent or non-absorbent. Preferably, the flexible extensions 24 have at least some absorbency. However, the majority of the fluid absorbed and retained by the absorbent interlabial device 20 will preferably ultimately be retained in the central absorbent portion 22. For a more detailed description of hydrophilicity and contact angles see the following publications which are incorporated by reference herein: The American Chemical Society Publication entitled "Contact Angle, Wettability, and Adhesion," edited by Robert F. Gould, and copyrighted in 1964; and TRI/Princeton Publications, Publication Number 459, entitled "A Microtechnique for Determining Surface Tension," published in April 1992, and Publication Number 468 entitled, "Determining Contact Angles Within Porous Networks," published in January, 1993, both edited by Dr. H. G. Heilweil.

The pleated design shown in FIGS. 1 and 2 has the additional benefit of easily providing the flexible extensions 24. The extensions 24 can comprise the same material as the central absorbent portion 22, or they can comprise a different material. The extensions 24 are joined to the upper portion 26 of the central

absorbent portion 22, and most preferably, for this embodiment, are joined to the top surface of the central absorbent portion 22, or within 1 millimeter of the top surface of the central absorbent portion 22. Preferably, in the embodiment shown in FIGS. 1 and 2, the extensions 24 are integral portions of the central absorbent portion 22 (that is, the extensions 24 comprise integral extensions of the absorbent tissue material that is folded to form the central absorbent portion 22.

The interlabial device 20 in any of the embodiments shown in the drawings may comprise other optional components. For example, the interlabial device 20 may comprise a topsheet 42 positioned over and joined to all or a portion of the body facing surface of the device 20 and/or a backsheet 38 positioned over and joined to all or a portion of its back surface, including the flexible extensions 24. Preferably, if a topsheet 42 and/or a backsheet 38 is used, these components are joined to at least a portion of the central absorbent portion. In an alternative embodiment, the central absorbent portion could be at least partially wrapped by a topsheet 42.

If a topsheet is used, the topsheet should be compliant, soft feeling, and non-irritating to the wearer's skin. Further, the topsheet should be liquid pervious permitting liquids (e.g., menses and/or urine) to readily penetrate through its thickness. A suitable topsheet may be manufactured from a wide range of materials such as woven and nonwoven materials comprised of natural fibers (e.g., wood or cotton fibers), synthetic fibers (e.g., polymeric fibers such as polyester, rayon, polypropylene, or polyethylene fibers) or from a combination of natural and synthetic fibers. Other woven and nonwoven materials may include polymeric materials such as apertured formed thermoplastic films, apertured plastic films, and hydroformed thermoplastic films; porous foams; reticulated foams; reticulated thermoplastic films; and thermoplastic scrims.

The topsheet may comprise an apertured formed film. Apertured formed films are pervious to body exudates and, if properly apertured, have a reduced tendency to allow liquids to pass back through and rewet the wearer's skin. Thus, the surface of the formed film which is in contact with the body remains dry, thereby reducing body soiling and creating a more comfortable feel for the wearer. Suitable formed films are described in U.S. Patent 3,929,135, entitled "Absorptive Structures Having Tapered Capillaries", which issued to Thompson on December 30, 1975; U.S. Patent 4,324,246 entitled "Disposable Absorbent Article Having A Stain Resistant Topsheet", which issued to Mullane, et al. on April 13, 1982; U.S. Patent 4,342,314 entitled "Resilient Plastic Web Exhibiting Fiber-Like Properties", which

issued to Radel, et al. on August 3, 1982; U.S. Patent 4,463,045 entitled "Macroscopically Expanded Three-Dimensional Plastic Web Exhibiting Non-Glossy Visible Surface and Cloth-Like Tactile Impression", which issued to Ahr, et al. on July 31, 1984; and U.S. 5,006,394 "Multilayer Polymeric Film" issued to Baird on April 9, 1991. The preferred topsheet for the interlabial device is the formed film described in one or more of the above patents and marketed on sanitary napkins by The Procter & Gamble Company of Cincinnati, Ohio as the "DRI-WEAVE" topsheet.

If such a formed film is used in an interlabial device, the body surface of the formed film topsheet is preferably hydrophilic so as to help liquid to transfer through the topsheet faster than if the body surface was not hydrophilic so as to diminish the likelihood that menstrual fluid will flow off the topsheet rather than flowing into and being absorbed by the central absorbent portion 22. In a preferred embodiment, surfactant is incorporated into the polymeric materials of the formed film topsheet. Alternatively, the body surface of the topsheet can be made hydrophilic by treating it with a surfactant such as is described in U.S. Patent 4,950,254 issued to Osborn.

If a backsheet is used, the backsheet 38 could be impervious or semi-pervious to liquids (e.g., menses and/or urine) and is preferably flexible. As used herein, the term "flexible" refers to materials which are compliant and will readily conform to the general shape and contours of the human body. The backsheet 38 prevents the exudates absorbed and contained in the central absorbent portion 22 from wetting articles which contact the absorbent interlabial device 20 such as the wearer's undergarments. The backsheet also assists the central absorbent portion 22 in preventing the wearer's body from being soiled by exudates. Additionally, use of the backsheet may provide an improved surface for the wearer to grasp between the fingers as the absorbent interlabial device 20 is inserted, or as the device is optionally removed with the fingers.

The backsheet 38 may comprise a woven or nonwoven material, polymeric films such as thermoplastic films of polyethylene or polypropylene, or composite materials such as a film-coated nonwoven material. Preferably, the backsheet 38 is a film having a thickness of from about 0.012 mm (0.5 mil) to about 0.051 mm (2.0 mils). An exemplary polyethylene film is manufactured by Clopay Corporation of Cincinnati, Ohio, under the designation P18-0401. The backsheet may permit vapors to escape from the central absorbent portion 22 (i.e., breathable) while still preventing exudates from passing through the backsheet.

The embodiments shown in FIGS. 1-3 and any other variations of such a type of device may be packaged in an individual package 60 as shown in FIG. 4. The individual package 60 comprises a wrapper 50 that encloses the absorbent interlabial device 20 to provide a sanitary environment. The wrapper 50 should at least partially enclose the absorbent interlabial device 20, and preferably completely enclose the absorbent interlabial device 20. The wrapper 50 preferably comprises a rectangular sheet of flexible material. The wrapper 50 can be folded about or wrapped around the absorbent interlabial device 20 in any suitable manner. The wrapper 50 is preferably folded about or wrapped around the absorbent interlabial device 20 with its longer sides oriented perpendicular to the longitudinal centerline L of the absorbent interlabial device 20.

In the preferred embodiment shown, the wrapping of the wrapper 50 forms a longitudinal fold or bend 58 around the lower longitudinal edge 29 of the absorbent interlabial device 20, opposing longitudinal edges 52, side edges 54, and side panels 68. The upper longitudinal edge 52, that is, the longitudinal edge closest to the upper portion of the absorbent interlabial device 20, and the side edges 54 are sealed to form the individual package 60. The upper longitudinal edge 52 and side edges 54 are preferably frangibly sealed together forming crimped edges 56 to close off the sides and ends of the package. Suitable methods for frangibly sealing the edges of a package are described in U.S. Patent 4,556,146 issued to Swanson, et al., U.S. Patent 5,181,610 issued to Quick, and U.S. Patent 5,462,166 issued to Minton, et al.

The individual package 60 preferably has a line of weakness which can be in the form of perforations 66 that are positioned along the upper longitudinal edge 52 and extend substantially along each side edge 54 of the package. In other alternate embodiments, the line of weakness can be in the form of a score line, such as that made by laser scoring. The individual package 60 preferably also has a tear strip or string 62 that generally extends along and in the direction of the perforations 66. The individual package 60 is opened by using the tear string 62 to break the perforations 66 along a significant portion of the periphery of the individual package 60. This releases two distinct side panels 68 which will drape over both sides of the user's fingers, and exposes the absorbent interlabial device 20.

The wrapper 50 is partially removable from around the device 20 and the portion of the wrapper 50 forming the longitudinal fold or bend 58 remains between the user's hand and the absorbent device 20 to assist in the positioning and placement of the device 20. This configuration assists the user in positioning and



placing the device 20, shields the user's fingers from being soiled, and keeps the user's fingers from touching the device 20 to maintain a sterile environment. FIG. 5 shows an opened individual package 60, as described above, with the interlabial device 20 being properly positioned in the folds of the labia.

5 In an alternative embodiment shown in FIG. 6, the individual package 60 is provided with a tab 64 instead of a tear string. The individual package 60 is opened by lifting the tab 64 and breaking the perforations 66 that are positioned along the upper portion of at least one side panel 68, that is closest to the upper portion of the absorbent interlabial device 20, to create an opening for the interlabial device 20.  
 10 The crimped edges 56 are pulled apart to release the side panels 68. The tab 64 is formed when an extension of the upper longitudinal edge 52 is folded over or bent over onto a side panel 68. The side edges 54 are sealed as described above. In yet another alternative embodiment, the wrapper 50 of any of the embodiments described herein can be formed with two separate sheets that are frangibly sealed  
 15 around the periphery of the sheets to form an individual package.

In an alternative embodiment shown in FIG. 7, the individual package 60 is provided with a side opening feature, such as a side tab 65 instead of a tear string. The side tab 65 preferably aligns with perforations 66 along the upper longitudinal edge of the package. The individual package 60 is opened by peeling back the side  
 20 tab 65 and breaking the perforations 66 that are positioned along the upper longitudinal edge 52 to expose the upper portion of the interlabial device 20. The crimped edges 56 are pulled apart to release the side panels 68. The package shown in FIG. 7 is otherwise similar to the package in FIG. 4 as described above. The side tab 65 may be formed in a number of ways, one of which removes material to form  
 25 the side tab 65 after the package has been sealed by cutting the desired pattern of the side tab 65. For example a notch 67 can be cut into the side edge 54 of the package to form the side tab 65. Another way to form the tab would be to precut the wrapper material prior to forming the individual package.

The absorbent interlabial devices 20 shown in FIGS. 1-3 provide a  
 30 convenient zone for grasping the product and inserting the interlabial device 20 into the space between the labia. The lower portion 28 of the central absorbent portion 22 can be grasped by the user, and held as the wrapper 50 is opened as described above. As shown in FIG. 5, the wrapper 50 is still in contact with the interlabial device 20, as the user places the interlabial device 20 into the space between the labia.  
 35 Preferably, the wrapper 50 remains in contact with the interlabial device 20 until the

device 20 is at least partially placed into the space between the labia for use. The wrapper 50 is then preferably removed.

5 An advantage of the present invention, as shown in FIG. 5, is that it protects the user's fingers from touching either the interlabial device 20 or her body at the point of insertion during insertion. The side panels 68 drape completely over both sides of the user's fingers to maintain a hygienic environment for inserting and placing the product. Another advantage of present invention is that it provides a protective covering for the interlabial device 20 during transport or storage of the product. Maintaining a hygienic environment for the interlabial device before and  
10 during use is vital to prevent transferring unsanitary particles to the interlabial space.

Alternatively, the embodiment shown in FIG. 7 can have perforations that are longitudinally positioned midway between the upper and lower longitudinal edges 52, and are located on both sides of the individual package. To open the package, the user would peel back and remove the upper portion of the wrapper and  
15 use the lower portion of the wrapper to grasp the lower portion 28 of the central absorbent portion 22. The wrapper would remain between the user's hand and the absorbent device 20, assist the user in positioning and placing the device 20, and keep the user's fingers from touching the device 20 to maintain a sterile environment.

20 Preferably, the wrapper 50 has a thickness of from about .0127 mm (0.5 mil) to about 0.127 mm (5.0 mils). The wrapper 50 may be made from plastic films, that may be thermoplastic, nonwoven materials, collagen films, paper tissues, or laminates of tissue and a film, nonwoven material and a film, or any of the foregoing types of material with a coating thereon. One embodiment of the present invention  
25 may be made from a low basis weight tissue that disintegrates in water. The low basis weight tissue can be made of carboxymethyl cellulose with wood pulp fibers and will disintegrate in water with a temperature of 75 °F (24 °C) in approximately 6 seconds; and disintegrate in water with a temperature of 50 °F in approximately 8 seconds. One such material is sold as DISSOLVO® WLD-35 water soluble purge  
30 dam material for gas-tungsten arc (TIG) welding by CMS Gilbreath Packaging Systems of Bensalem, PA.

In addition, such low basis weight tissues may be combined with coatings or films like polyvinyl acetate (PVA), polyvinyl alcohol (PVOH), or methyl hydroxy propyl cellulose (MHPC) that also dissolve in water. One such material is sold as

Mono-Sol<sup>®</sup> MC-8630 water soluble film by Chris Craft<sup>®</sup> Industrial Products, Inc., Gary, IN. One preferred laminate material is made using a Hot Roll Laminator obtained from ChemInstruments by combining a .089 mm (3.5 mil) thick sheet of DISSOLVO<sup>®</sup> WLD-35 tissue with a .038 mm (1.5 mil) Mono-Sol<sup>®</sup> MC-8630 MHPC water soluble film. Laminating the tissue at a temperature between 344 °F (173 °C) to 366°F (185 °C) and at a feed rate between 35 ft/min to 50 ft/min with the MHPC film produces a material 0.1 mm (4 mil) thick that is preferred for making the wrapper of the present invention.

The laminated material has a basis weight of 93.6 g/m<sup>2</sup>. The material will disintegrate in water with a temperature of 75 °F (24 °C) in approximately 6.1 seconds and 7.9 seconds in water with a temperature of 50 °F. The average time for the laminated material to dissolve is approximately 17.3 seconds in water with a temperature 75 °F (24 °C) and 34.4 seconds in water with a temperature 50 °F (10 °C).

The tear resistance (tear strength) of the film is alone is approximately 1575 gf, while the tear resistance of the DISSOLVO<sup>®</sup> WLD-35 is approximately 25 gf in the direction of the process flow through a manufacturing line for making the paper, the machine direction (MD), and 25 gf in the direction perpendicular to the machine direction, the cross-machine direction (CD). The tear resistance of the laminated material is approximately 88 gf (MD), and 76.8 gf (CD). The tear strength of the laminate is significantly less than that of the film by itself. The increase in the tear strength when comparing the paper to the laminated material provides a stronger package that will not tear as easily as paper alone. The reduction in tear strength when comparing the film to the laminated paper and film enables the user to open the package with greater ease than if the package were made from the film alone. When the materials are laminated, the superior tear resistant properties of the film are compromised, yet the strength of the paper is significantly increased, providing an ideal package that is easily opened, yet strong enough to resist tearing from handling and transporting.

The laminated material, like a number of the other wrapper materials identified above, also aids in heat sealing the package, provides a sanitary and moisture-free environment, and reduces noise associated with tearing paper when opening and carrying the package. The laminated material also produces a wrapper that can be opened with or without a line of weakness.

The coated side of the paper can either face the product or serve as the outer portion of the wrapper that is touched by the user. The coated side can be placed adjacent to the interlabial device 20 to protect against moisture. When the coating is applied or laminated to the wrapper material as a continuous film it forms a nonporous, impervious barrier that blocks moisture. However, placing the non-coated side of the wrapper 50 adjacent to the interlabial device 20 provides an absorbent surface on the inside surface of the side panels 68, that when the product is opened, can be used to absorb and wipe away discharge that may be found on the labia or interlabial space when inserting the interlabial device 20.

The wrapper 50 is preferably constructed of material that aids in providing comfort during insertion. The laminated material, like a number of the other wrapper materials identified above, provides a softer wrapper material. The wrapper 50 is preferably constructed of materials which are at least 70% biodegradable, more preferably at least 90% biodegradable, and/or which will fragment in water with agitation (as in a toilet). Preferably, the absorbent interlabial device 20 and the wrapper 50 for the absorbent interlabial device are both flushable separately or in combination, and when flushed the wrapper or the combination of the absorbent interlabial product and the wrapper will clear the toilet 80% of the time and biodegrade at least 95% of the time in a 28 Day Sludge Test. As used herein the terms "flushable and flushability" refer to a an article's ability to pass through typical commercially available U.S. household toilets and plumbing drainage systems without causing clogging or similar problems that can be directly associated with the physical structure of the article.

It is recognized, however, that there can be many differences between the various types of toilets available. Therefore, for the purposes of the appended claims, a test to determine the flushability of a catamenial product, such as an interlabial device, or the wrapper of a catamenial product is set out in the TEST METHODS section of this specification.

In addition, numerous embodiments of the individual packages described herein are possible. For example, the package could be provided in other configurations while still performing the functions described herein. Further, the packaging materials described herein can be used with a variety of absorbent articles configured for the absorption of body fluids such as female or male incontinence products, tampons, or externally worn sanitary napkins where a hygienic environment is a paramount concern. For instance, the adhesive on sanitary napkins

and/or the wing adhesive of winged sanitary napkins can be covered by cover strips made of such materials. Additionally, a wrapper that serves as an individual package for a sanitary napkin such as that described in U.S. Patent 4,556,146 entitled "Individually Packaged Disposable Absorbent Article" which issued to Swanson et al. on December 3, 1985 could be provided that is made of such a material and/or have an absorbent inside surface which serves as a sanitary wiping device.

## TEST METHODS

### Flushability

#### 10 Overview

As noted above, the terms "flushable or flushability" refer to a article's capacity to pass through typical commercially available household toilets and plumbing drainage systems without causing clogging or similar problems that can be directly associated with the physical characteristics of the article. For the purpose of the  
15 appended claims, interlabial products and their wrappers are evaluated for flushability via relative ease of toilet bowl and trap evacuation and subsequent transport through a simulated plumbing system. The flushability of such an article should be measured by the following test procedure.

The test procedure is designed to simulate two days of normal toilet usage for a  
20 family of 4 (2 men, 2 women). The test employs a flushing sequence to simulate the following conditions: male urination visits, female urination visits (including post urinary drying with tissue), disposal of the interlabial product or wrapper with cleaning using tissue, and bowel movement visits. The amount of tissue to be used for each tissue flush is a normal loading of 2 strips of seven sheets. The normal  
25 loading is based on consumer research regarding typical habits and practices. The test is designed to simulate the conditions an article will encounter if it is flushed through a conventional toilet and into a municipal sewer or into a septic tank. Samples are evaluated for: 1) toilet bowl and trap clearance, 2) drain line blockage, and 3) disintegration during flushing.

#### 30 Apparatus

An apparatus suitable for the flushability test is shown in plan view in Figure 9. The apparatus includes:

- a 3.5 gallon (13.2 liter) water saver siphon vortex toilet referred to as 210 (additional toilets can also be attached to the piping layout shown in FIG. 9 to evaluate the behavior of test samples using different flushing mechanisms such as commercial, pressure toilets);
- 5 • approximately 59 feet (18 meters) of 4 inch (10 cm) inside diameter acrylic pipe (As can be seen from FIG. 9, the piping is assembled in roughly a square configuration having linear runs 211, 213, 215, 217, 219, 221 approximately 10 feet (3 meters) long);
- 10 • a cast iron tee 223 slightly downstream of the toilet 210 that is open to the atmosphere for venting;
- five cast iron ninety degree elbows 212, 214, 216, 218, and 220;
- a spike or snag 222 positioned vertically (FIG. 10) approximately 15 feet from the pipe's terminal end and approximately 1 inch (2.5 cm) long; and
- 15 • a screen 224 (No. 4 Tyler sieve) to capture solid effluent for evaluation of disintegration.

The apparatus used for this method is set up to be equivalent to ANSI Standard A112.19.2M-1990 for Vitreous China fixtures. The piping is plumbed to provide a drop of 0.25 inch per foot (2 centimeters/meter) of pipe length.

#### Materials

- 20 Tissue Product used in Test: Standard CHARMIN® toilet tissue manufactured by The Procter & Gamble Company of Cincinnati, Ohio.

Synthetic Fecal Material: Prepared according to the method described below

#### Test Flushing Sequence

- 25 The test flushing sequence, consisting of two routines, simulates 2 days of normal toilet usage for a family of 4 (2 men, 2 women; based on consumer habits and practices research). The sequence of 40 total flushes consists of 14 flushes with an empty bowl; 8 flushes with tissue only; 6 flushes with tissue and wrapper; 6 flushes with tissue, interlabial product and wrapper; and 6 flushes with tissue and simulated fecal matter (SFM). When testing the wrapper and interlabial product as a
- 30 combination, perform routines 1 and 2 using both the wrapper and the interlabial

product placed individually into the bowl by first removing the product from the wrapper. The SFM, when it is used, is placed in the bowl just prior to the addition of tissue. The SFM loading of  $160 \text{ g} \pm 5 \text{ g}$  consists of two 1 inch (2.5 centimeter) x 4 inch (10 centimeter) pieces and one 1 inch (2.5 centimeter) x 2 inch (5 centimeter) piece. 5  
 10  
 15  
 20  
 25  
 30  
 35  
 40  
 45  
 50  
 55  
 60  
 65  
 70  
 75  
 80  
 85  
 90  
 95  
 100  
 105  
 110  
 115  
 120  
 125  
 130  
 135  
 140  
 145  
 150  
 155  
 160  
 165  
 170  
 175  
 180  
 185  
 190  
 195  
 200  
 205  
 210  
 215  
 220  
 225  
 230  
 235  
 240  
 245  
 250  
 255  
 260  
 265  
 270  
 275  
 280  
 285  
 290  
 295  
 300  
 305  
 310  
 315  
 320  
 325  
 330  
 335  
 340  
 345  
 350  
 355  
 360  
 365  
 370  
 375  
 380  
 385  
 390  
 395  
 400  
 405  
 410  
 415  
 420  
 425  
 430  
 435  
 440  
 445  
 450  
 455  
 460  
 465  
 470  
 475  
 480  
 485  
 490  
 495  
 500  
 505  
 510  
 515  
 520  
 525  
 530  
 535  
 540  
 545  
 550  
 555  
 560  
 565  
 570  
 575  
 580  
 585  
 590  
 595  
 600  
 605  
 610  
 615  
 620  
 625  
 630  
 635  
 640  
 645  
 650  
 655  
 660  
 665  
 670  
 675  
 680  
 685  
 690  
 695  
 700  
 705  
 710  
 715  
 720  
 725  
 730  
 735  
 740  
 745  
 750  
 755  
 760  
 765  
 770  
 775  
 780  
 785  
 790  
 795  
 800  
 805  
 810  
 815  
 820  
 825  
 830  
 835  
 840  
 845  
 850  
 855  
 860  
 865  
 870  
 875  
 880  
 885  
 890  
 895  
 900  
 905  
 910  
 915  
 920  
 925  
 930  
 935  
 940  
 945  
 950  
 955  
 960  
 965  
 970  
 975  
 980  
 985  
 990  
 995  
 1000  
 1005  
 1010  
 1015  
 1020  
 1025  
 1030  
 1035  
 1040  
 1045  
 1050  
 1055  
 1060  
 1065  
 1070  
 1075  
 1080  
 1085  
 1090  
 1095  
 1100  
 1105  
 1110  
 1115  
 1120  
 1125  
 1130  
 1135  
 1140  
 1145  
 1150  
 1155  
 1160  
 1165  
 1170  
 1175  
 1180  
 1185  
 1190  
 1195  
 1200  
 1205  
 1210  
 1215  
 1220  
 1225  
 1230  
 1235  
 1240  
 1245  
 1250  
 1255  
 1260  
 1265  
 1270  
 1275  
 1280  
 1285  
 1290  
 1295  
 1300  
 1305  
 1310  
 1315  
 1320  
 1325  
 1330  
 1335  
 1340  
 1345  
 1350  
 1355  
 1360  
 1365  
 1370  
 1375  
 1380  
 1385  
 1390  
 1395  
 1400  
 1405  
 1410  
 1415  
 1420  
 1425  
 1430  
 1435  
 1440  
 1445  
 1450  
 1455  
 1460  
 1465  
 1470  
 1475  
 1480  
 1485  
 1490  
 1495  
 1500  
 1505  
 1510  
 1515  
 1520  
 1525  
 1530  
 1535  
 1540  
 1545  
 1550  
 1555  
 1560  
 1565  
 1570  
 1575  
 1580  
 1585  
 1590  
 1595  
 1600  
 1605  
 1610  
 1615  
 1620  
 1625  
 1630  
 1635  
 1640  
 1645  
 1650  
 1655  
 1660  
 1665  
 1670  
 1675  
 1680  
 1685  
 1690  
 1695  
 1700  
 1705  
 1710  
 1715  
 1720  
 1725  
 1730  
 1735  
 1740  
 1745  
 1750  
 1755  
 1760  
 1765  
 1770  
 1775  
 1780  
 1785  
 1790  
 1795  
 1800  
 1805  
 1810  
 1815  
 1820  
 1825  
 1830  
 1835  
 1840  
 1845  
 1850  
 1855  
 1860  
 1865  
 1870  
 1875  
 1880  
 1885  
 1890  
 1895  
 1900  
 1905  
 1910  
 1915  
 1920  
 1925  
 1930  
 1935  
 1940  
 1945  
 1950  
 1955  
 1960  
 1965  
 1970  
 1975  
 1980  
 1985  
 1990  
 1995  
 2000  
 2005  
 2010  
 2015  
 2020  
 2025  
 2030  
 2035  
 2040  
 2045  
 2050  
 2055  
 2060  
 2065  
 2070  
 2075  
 2080  
 2085  
 2090  
 2095  
 2100  
 2105  
 2110  
 2115  
 2120  
 2125  
 2130  
 2135  
 2140  
 2145  
 2150  
 2155  
 2160  
 2165  
 2170  
 2175  
 2180  
 2185  
 2190  
 2195  
 2200  
 2205  
 2210  
 2215  
 2220  
 2225  
 2230  
 2235  
 2240  
 2245  
 2250  
 2255  
 2260  
 2265  
 2270  
 2275  
 2280  
 2285  
 2290  
 2295  
 2300  
 2305  
 2310  
 2315  
 2320  
 2325  
 2330  
 2335  
 2340  
 2345  
 2350  
 2355  
 2360  
 2365  
 2370  
 2375  
 2380  
 2385  
 2390  
 2395  
 2400  
 2405  
 2410  
 2415  
 2420  
 2425  
 2430  
 2435  
 2440  
 2445  
 2450  
 2455  
 2460  
 2465  
 2470  
 2475  
 2480  
 2485  
 2490  
 2495  
 2500  
 2505  
 2510  
 2515  
 2520  
 2525  
 2530  
 2535  
 2540  
 2545  
 2550  
 2555  
 2560  
 2565  
 2570  
 2575  
 2580  
 2585  
 2590  
 2595  
 2600  
 2605  
 2610  
 2615  
 2620  
 2625  
 2630  
 2635  
 2640  
 2645  
 2650  
 2655  
 2660  
 2665  
 2670  
 2675  
 2680  
 2685  
 2690  
 2695  
 2700  
 2705  
 2710  
 2715  
 2720  
 2725  
 2730  
 2735  
 2740  
 2745  
 2750  
 2755  
 2760  
 2765  
 2770  
 2775  
 2780  
 2785  
 2790  
 2795  
 2800  
 2805  
 2810  
 2815  
 2820  
 2825  
 2830  
 2835  
 2840  
 2845  
 2850  
 2855  
 2860  
 2865  
 2870  
 2875  
 2880  
 2885  
 2890  
 2895  
 2900  
 2905  
 2910  
 2915  
 2920  
 2925  
 2930  
 2935  
 2940  
 2945  
 2950  
 2955  
 2960  
 2965  
 2970  
 2975  
 2980  
 2985  
 2990  
 2995  
 3000  
 3005  
 3010  
 3015  
 3020  
 3025  
 3030  
 3035  
 3040  
 3045  
 3050  
 3055  
 3060  
 3065  
 3070  
 3075  
 3080  
 3085  
 3090  
 3095  
 3100  
 3105  
 3110  
 3115  
 3120  
 3125  
 3130  
 3135  
 3140  
 3145  
 3150  
 3155  
 3160  
 3165  
 3170  
 3175  
 3180  
 3185  
 3190  
 3195  
 3200  
 3205  
 3210  
 3215  
 3220  
 3225  
 3230  
 3235  
 3240  
 3245  
 3250  
 3255  
 3260  
 3265  
 3270  
 3275  
 3280  
 3285  
 3290  
 3295  
 3300  
 3305  
 3310  
 3315  
 3320  
 3325  
 3330  
 3335  
 3340  
 3345  
 3350  
 3355  
 3360  
 3365  
 3370  
 3375  
 3380  
 3385  
 3390  
 3395  
 3400  
 3405  
 3410  
 3415  
 3420  
 3425  
 3430  
 3435  
 3440  
 3445  
 3450  
 3455  
 3460  
 3465  
 3470  
 3475  
 3480  
 3485  
 3490  
 3495  
 3500  
 3505  
 3510  
 3515  
 3520  
 3525  
 3530  
 3535  
 3540  
 3545  
 3550  
 3555  
 3560  
 3565  
 3570  
 3575  
 3580  
 3585  
 3590  
 3595  
 3600  
 3605  
 3610  
 3615  
 3620  
 3625  
 3630  
 3635  
 3640  
 3645  
 3650  
 3655  
 3660  
 3665  
 3670  
 3675  
 3680  
 3685  
 3690  
 3695  
 3700  
 3705  
 3710  
 3715  
 3720  
 3725  
 3730  
 3735  
 3740  
 3745  
 3750  
 3755  
 3760  
 3765  
 3770  
 3775  
 3780  
 3785  
 3790  
 3795  
 3800  
 3805  
 3810  
 3815  
 3820  
 3825  
 3830  
 3835  
 3840  
 3845  
 3850  
 3855  
 3860  
 3865  
 3870  
 3875  
 3880  
 3885  
 3890  
 3895  
 3900  
 3905  
 3910  
 3915  
 3920  
 3925  
 3930  
 3935  
 3940  
 3945  
 3950  
 3955  
 3960  
 3965  
 3970  
 3975  
 3980  
 3985  
 3990  
 3995  
 4000  
 4005  
 4010  
 4015  
 4020  
 4025  
 4030  
 4035  
 4040  
 4045  
 4050  
 4055  
 4060  
 4065  
 4070  
 4075  
 4080  
 4085  
 4090  
 4095  
 4100  
 4105  
 4110  
 4115  
 4120  
 4125  
 4130  
 4135  
 4140  
 4145  
 4150  
 4155  
 4160  
 4165  
 4170  
 4175  
 4180  
 4185  
 4190  
 4195  
 4200  
 4205  
 4210  
 4215  
 4220  
 4225  
 4230  
 4235  
 4240  
 4245  
 4250  
 4255  
 4260  
 4265  
 4270  
 4275  
 4280  
 4285  
 4290  
 4295  
 4300  
 4305  
 4310  
 4315  
 4320  
 4325  
 4330  
 4335  
 4340  
 4345  
 4350  
 4355  
 4360  
 4365  
 4370  
 4375  
 4380  
 4385  
 4390  
 4395  
 4400  
 4405  
 4410  
 4415  
 4420  
 4425  
 4430  
 4435  
 4440  
 4445  
 4450  
 4455  
 4460  
 4465  
 4470  
 4475  
 4480  
 4485  
 4490  
 4495  
 4500  
 4505  
 4510  
 4515  
 4520  
 4525  
 4530  
 4535  
 4540  
 4545  
 4550  
 4555  
 4560  
 4565  
 4570  
 4575  
 4580  
 4585  
 4590  
 4595  
 4600  
 4605  
 4610  
 4615  
 4620  
 4625  
 4630  
 4635  
 4640  
 4645  
 4650  
 4655  
 4660  
 4665  
 4670  
 4675  
 4680  
 4685  
 4690  
 4695  
 4700  
 4705  
 4710  
 4715  
 4720  
 4725  
 4730  
 4735  
 4740  
 4745  
 4750  
 4755  
 4760  
 4765  
 4770  
 4775  
 4780  
 4785  
 4790  
 4795  
 4800  
 4805  
 4810  
 4815  
 4820  
 4825  
 4830  
 4835  
 4840  
 4845  
 4850  
 4855  
 4860  
 4865  
 4870  
 4875  
 4880  
 4885  
 4890  
 4895  
 4900  
 4905  
 4910  
 4915  
 4920  
 4925  
 4930  
 4935  
 4940  
 4945  
 4950  
 4955  
 4960  
 4965  
 4970  
 4975  
 4980  
 4985  
 4990  
 4995  
 5000  
 5005  
 5010  
 5015  
 5020  
 5025  
 5030  
 5035  
 5040  
 5045  
 5050  
 5055  
 5060  
 5065  
 5070  
 5075  
 5080  
 5085  
 5090  
 5095  
 5100  
 5105  
 5110  
 5115  
 5120  
 5125  
 5130  
 5135  
 5140  
 5145  
 5150  
 5155  
 5160  
 5165  
 5170  
 5175  
 5180  
 5185  
 5190  
 5195  
 5200  
 5205  
 5210  
 5215  
 5220  
 5225  
 5230  
 5235  
 5240  
 5245  
 5250  
 5255  
 5260  
 5265  
 5270  
 5275  
 5280  
 5285  
 5290  
 5295  
 5300  
 5305  
 5310  
 5315  
 5320  
 5325  
 5330  
 5335  
 5340  
 5345  
 5350  
 5355  
 5360  
 5365  
 5370  
 5375  
 5380  
 5385  
 5390  
 5395  
 5400  
 5405  
 5410  
 5415  
 5420  
 5425  
 5430  
 5435  
 5440  
 5445  
 5450  
 5455  
 5460  
 5465  
 5470  
 5475  
 5480  
 5485  
 5490  
 5495  
 5500  
 5505  
 5510  
 5515  
 5520  
 5525  
 5530  
 5535  
 5540  
 5545  
 5550  
 5555  
 5560  
 5565  
 5570  
 5575  
 5580  
 5585  
 5590  
 5595  
 5600  
 5605  
 5610  
 5615  
 5620  
 5625  
 5630  
 5635  
 5640  
 5645  
 5650  
 5655  
 5660  
 5665  
 5670  
 5675  
 5680  
 5685  
 5690  
 5695  
 5700  
 5705  
 5710  
 5715  
 5720  
 5725  
 5730  
 5735  
 5740  
 5745  
 5750  
 5755  
 5760  
 5765  
 5770  
 5775  
 5780  
 5785  
 5790  
 5795  
 5800  
 5805  
 5810  
 5815  
 5820  
 5825  
 5830  
 5835  
 5840  
 5845  
 5850  
 5855  
 5860  
 5865  
 5870  
 5875  
 5880  
 5885  
 5890  
 5895  
 5900  
 5905  
 5910  
 5915  
 5920  
 5925  
 5930  
 5935  
 5940  
 5945  
 5950  
 5955  
 5960  
 5965  
 5970  
 5975  
 5980  
 5985  
 5990  
 5995  
 6000  
 6005  
 6010  
 6015  
 6020  
 6025  
 6030  
 6035  
 6040  
 6045  
 6050  
 6055  
 6060  
 6065  
 6070  
 6075  
 6080  
 6085  
 6090  
 6095  
 6100  
 6105  
 6110  
 6115  
 6120  
 6125  
 6130  
 6135  
 6140  
 6145  
 6150  
 6155  
 6160  
 6165  
 6170  
 6175  
 6180  
 6185  
 6190  
 6195  
 6200  
 6205  
 6210  
 6215  
 6220  
 6225  
 6230  
 6235  
 6240  
 6245  
 6250  
 6255  
 6260  
 6265  
 6270  
 6275  
 6280  
 6285  
 6290  
 6295  
 6300  
 6305  
 6310  
 6315  
 6320  
 6325  
 6330  
 6335  
 6340  
 6345  
 6350  
 6355  
 6360  
 6365  
 6370  
 6375  
 6380  
 6385  
 6390  
 6395  
 6400  
 6405  
 6410  
 6415  
 6420  
 6425  
 6430  
 6435  
 6440  
 6445  
 6450  
 6455  
 6460  
 6465  
 6470  
 6475  
 6480  
 6485  
 6490  
 6495  
 6500  
 6505  
 6510  
 6515  
 6520  
 6525  
 6530  
 6535  
 6540  
 6545  
 6550  
 6555  
 6560  
 6565  
 6570  
 6575  
 6580  
 6585  
 6590  
 6595  
 6600  
 6605  
 6610  
 6615  
 6620  
 6625  
 6630  
 6635  
 6640  
 6645  
 6650  
 6655  
 6660  
 6665  
 6670  
 6675  
 6680  
 6685  
 6690  
 6695  
 6700  
 6705  
 6710  
 6715  
 6720  
 6725  
 6730  
 6735  
 6740  
 6745  
 6750  
 6755  
 6760  
 6765  
 6770  
 6775  
 6780  
 6785  
 6790  
 6795  
 6800  
 6805  
 6810  
 6815  
 6820  
 6825  
 6830  
 6835  
 6840  
 6845  
 6850  
 6855  
 6860  
 6865  
 6870  
 6875  
 6880  
 6885  
 6890  
 6895  
 6900  
 6905  
 6

- 2) Flush With Empty Bowl. Take a drain line blockage reading 2 minutes after the water reaches the snag point and move to step 3.
- 3) Flush With Tissue Only - Take a drain line blockage reading 2 minutes after the water reaches the snag point, wait 1 additional minute, and move to step 4.
- 4) Flush With Empty Bowl. Take a drain line blockage reading 2 minutes after the water reaches the snag point.

Total number of flushes for the sequence (Routine 1 + Routine 2) is 40.

If, after the second flush in the flushing sequence, the product remains in the bowl or trap after flushing, the tissue and or catamenial product and or wrapper is plunged into the drainage line manually and the flushing sequence will continue. After completion of each trial loading, the drainage pipe will be cleared prior to beginning subsequent testing.

The above described flushing sequence is repeated three times for each test product.

#### Data Reporting

The degree of drain line blockage is determined by measuring the length of water dammed up behind the obstruction. Graduations are marked every 12 inches (30 centimeters) on the drainpipe upstream of the obstruction. Each one foot length that the water is backed up corresponds to 0.25 inch (0.6 centimeter) or 6.25% of blockage at the obstruction point. Test product residues which exit the drainpipe are also collected.

The following data are recorded for each evaluation:

- 1) Incidence of failure (%) of wrapper to clear bowl and trap in one flush
- 2) Incidence of failure (%) of wrapper to clear bowl and trap in two flushes
- 3) Incidence of wrapper on simulated snag



4) Maximum level (%) of drain line blockage

5) Cumulative level (%) of drain line blockage over the 2 day simulated test period.

Preferably, the wrapper described herein will completely clear the bowl at least about 70% of the time in two or fewer flushes, more preferably at least about 80% of the time in one flush, and most preferably at least about 95% of the time in one flush. The wrapper described herein will preferably have a maximum level of drain line blockage of less than or equal to about 80%. The wrapper described herein will preferably have a cumulative level of drain line blockage over the 2 day simulated test period of less than or equal to about 50%.

#### Preparation of Synthetic Fecal Material

##### I. Materials Needed:

- Feclone synthetic fecal matter (900 grams);  
(Available from Siliclone Studio, Valley Forge, PA as product BFPS-7 dry concentrate)
- Tap water at 100° C (6066 grams)

##### II. Equipment Needed:

- Mixer (Available from Hobart Corp., Troy, OH as Model A200)
- Extruder (Available from Hobart Corp., Troy, OH as Model 4812)
- Disposable Centrifuge tubes with screw caps (50 ml) (Available from VWR Scientific, Chicago, IL as Catalog No. 21-008-176)
- Water Bath to control temperature to 37° C.

##### III. Preparation:

1. Pour the 100° C water into the mixing bowl of the mixer and add the dry Feclone concentrate.

2. Mix on low for 1 minute.
3. Mix on medium speed for 2 minutes.
4. After the material is well mixed, transfer to the extruder.
5. Using an ice pick, punch a small hole in the tip of each centrifuge tube.
6. Extrude the Feclone into the centrifuge tubes.
7. Cap the centrifuge tubes and store in the refrigerator.
8. Before using, put the tubes in the water bath at 38° C.

10

### Water Dispersion Test

#### Apparatus

15

**Stirrer** Magnetic, Thermolyne type Model S7225 or 7200. Permanently inscribe a circle 3.5 inches (8.9 centimeter) on the top surface of the stirrer. The center of the circle must be coincident with the geometric center of the stirrer.

**Stirring Bar** 2.5 inch (6.2 centimeter) TEFLON coated with spinning ring. Permanently mark one end of the bar with black ink for a distance of 0.5 inch (1.2 centimeter) back from the tip.

**Thermometer** 30 to 120°F with 1 degree divisions

20

**Timer** Digital stopwatch

**Stroboscope** Variable speed stroboscope, model 964 available from Strobette, Power Instrument, Inc. of Skokie, IL is suitable

25

**Beaker** Kimax brand 2000 milliliter with spout with a diameter at the base of  $135 \pm 2$  mm and a height at the 2000ml mark of  $162 \pm 2$  mm, Inscribe a fill mark at a height of 5.6 inches (14.3 centimeters) from the flat bottom of the beaker. Do not use any beaker not having a flat bottom.

Conditioned Room: Temperature and humidity should be controlled to remain within the following limits:

Temperature:  $73 \pm 3^{\circ}\text{F}$  ( $23^{\circ}\text{C} \pm 2^{\circ}\text{C}$ )

Humidity:  $50 \pm 2\%$  Relative Humidity

## 5 Test Setup

1. Fill the beaker to the fill mark with  $73 \pm 3^{\circ}\text{F}$  ( $23^{\circ}\text{C} \pm 2^{\circ}\text{C}$ ) tap water.
2. Place the beaker on the magnetic stirrer centering it in the inscribed circle.
- 10 3. Add the stirring bar to the beaker.
4. Turn the stroboscope on and set the speed to 1000 rpm according to the manufacturer's directions.
5. Turn the magnetic stirrer on with the on/off switch. Adjust the speed of the magnetic stirrer until the stirring bar appears to be stationary and both ends appear to be black. This indicates that the magnetic stirrer is turning at 500 rpm (i.e. half the setting on the stroboscope). Turn the magnetic stirrer off with the on/off switch.

15

## Procedure

- 20 1. Hold a sample (e.g. an absorbent interlabial device or wrapper) 3 to 4 inches (7.6 to 10.2 centimeters) above the surface of the water. Gently drop the sample onto the water surface, starting the timer when the sample touches the water surface.
2. Wait 5 seconds.
- 25 3. Start the magnetic stirrer with the on/off switch. If the sample disrupts the rotation of the stirring bar, stop the stirrer, re-orient the bar, and immediately start the stirrer again.

4. Record the time required until the sample separates into at least two pieces. Separation does not include the disassociation of a few individual fibers from an otherwise intact sample. The time is the total time the sample is immersed in the water including the time the stirrer may have been stopped to re-orient the sample.

5. A circular wire screen, consisting of an outer circle of 3" (7.62 cm) diameter and equally divided into 6 sections made from copper wire about 1mm in diameter, may be placed immediately suspended above the stir bar in cases where the wrapper substantially disrupts the rotation of the stir bar.

10. If the wrapper repeatedly causes substantial disruption to the rotation of the stirring bar, the wrapper may be suspended by a string attached to the wrapper via a clamp attached to the wrapper 3/8" (.95 cm) from the edge of the wrapper, and then suspending the lowest end of the wrapper 1" above the stir bar.

15. 5. Repeat steps 1 through 4 with an additional 3 samples.

## 20. Calculation and Reporting

Calculate and report the mean and standard deviation of the water dispersibility time for the four samples tested. Preferably, the wrapper will disperse into at least two fragments in less than or equal to about two hours.

### Wet-Out Time

25. 1. Hold the absorbent interlabial device or wrapper 3 to 4 inches (7.62 to 10.16 cm) above the surface of distilled water.
2. Gently drop the sample onto the water surface, so that the broad surface of the package strikes the surface.
3. Start timing when the sample is completely wet.
30. 4. Repeat steps 1-2 for five samples.

Report a mean and standard deviation for the wet-out time. The wet-out time is preferably less than or equal to 30 seconds and more preferably less than or equal to 15 seconds.

### 28 Day Sludge Test

#### Purpose:

To determine the extent to which a wrapper disintegrates upon exposure to biologically active anaerobic sludge. Anaerobic conditions are typically found in household septic tanks, as well as in municipal sewage treatment facilities in the form of anaerobic sludge digesters. Test products, such as the wrapper are combined with anaerobic digester sludge to determine the extent and rate of disintegration of test products over a 28 day period. Disintegration (as measured by weight change) is typically measured on days 3, 7, 14, 21 and 28 of the particular study. This protocol is modeled after the National Sanitation Foundation, Ann Arbor, Michigan, International Protocol: Evaluation of the Anaerobic Disintegration of a Test Product, November, 1992.

#### Materials:

##### Control Product

Tampax brand tampons will be used as a positive control product in the anaerobic disintegration test.

##### Material Preparation

Prior to the addition of the test and control products to the reactors, the materials will be dried in a hot air oven at  $103^{\circ} \pm 2^{\circ}\text{C}$  for 2 hours and then weighed to determine the initial weight. Approximately equal weights of the control and test products will be placed in respective reactors.

##### Anaerobic Sludge:

The sludge used in this evaluation will be anaerobic sludge obtained from a municipal waste water treatment plant, or raw sewage obtained as influent from a

waste water treatment plant that has been concentrated by settling and decanting the overlying water. Prior to use in the evaluation, the following parameters of the sludge will be measured in accordance with standard laboratory operating procedures:

- 5           Total solids
- Total volatile solids
- pH

The sludge should meet the following criteria for use in the evaluation:

- pH between 6.5 and 8
- 10       Total solids  $\geq 15,000$  mg/L
- Total volatile solids  $\geq 10,000$  mg/L

The criteria for the activity of the sludge requires that the control tampon material must lose at least 95% of its initial dry weight after 28 days exposure.

15

#### Procedure:

- The test and control products are added to a 2L wide mouth glass flask (reactor) containing 1500 ml of anaerobic digester sludge or concentrated raw sewage. Three reactor flasks per test material per sampling day are prepared. Thus, if disintegration
- 20   is measured on days 3, 7, 14, 21, and 28, there will be a total of 15 reactor flasks for the test product and 15 flasks for the control product. The reactors are sealed and placed in an incubator maintained at  $35 \pm 2^\circ\text{C}$ . On the specified sampling days, three reactors each for the test and control material are removed from the incubator. On the designated sample days, the contents of each reactor will be passed through a 1
- 25   mm mesh screen to recover any undisintegrated material. Any collected material will be rinsed with tap water, removed from the screen and placed in a hot air oven at  $103 \pm 2^\circ\text{C}$  for at least 2 hours. The dried material will be weighed to determine final weight. Visual observations of the physical appearance of the materials when recovered from the reactors will also be made and recorded.

Results:

The rate and extent of anaerobic disintegration of each test material and the control material is determined from initial dry weights of the material and the dried weights of the material recovered on the sampling days. The percent anaerobic disintegration is determined using the following equation (percent weight loss):

$$\text{Percent Disintegration} = \frac{(\text{initial dry weight} - \text{final dry weight})}{(\text{initial dry weight})} \times 100$$

The average percent disintegration for the test and control products for each sampling day will be presented. For the purposes of the appended claims, the percent disintegration values are for day 28 of the study.

The disclosure of all patents, patent applications (and any patents which issue thereon, as well as any corresponding published foreign patent applications), and publications mentioned throughout this description are hereby incorporated by reference herein. It is expressly not admitted, however, that any of the documents incorporated by reference herein teach or disclose the present invention.

While particular embodiments of the present invention have been illustrated and described, it would be obvious to those skilled in the art that various other changes and modifications can be made without departing from the spirit and scope of the invention.

## WHAT IS CLAIMED IS:





1. An individual package for an absorbent interlabial device, wherein said absorbent interlabial device is to be inserted at least partially within a user's interlabial space, said individual package comprising:  
5 a wrapper for packaging said absorbent interlabial device, said wrapper comprising a flexible sheet which is at least partially wrapped around said absorbent interlabial device, said flexible sheet has an absorbent inside surface adjacent to said absorbent interlabial device, which when said wrapper is opened, provides the user with a sanitary wiping device to wipe  
10 the labia while inserting said absorbent interlabial device into the interlabial space.
2. The individual package of Claim 1 wherein said wrapper comprises at least one of the materials selected from the group consisting of: tissue; collagen  
15 film; thermoplastic film; nonwoven material; laminates of thermoplastic film and tissue; laminates of collagen film and tissue; laminates of thermoplastic film and nonwoven material; and laminates of collagen film and thermoplastic film.
3. The individual package of Claim 1 wherein said wrapper has an outside  
20 surface, and said outside surface is liquid impervious.
4. The individual package of Claim 1 that is sufficiently flushable that it completely clears the bowl under the Flushability Test at least 70% of the time in two or fewer flushes.
5. The individual package of Claim 1 that is sufficiently flushable that it  
25 completely clears the bowl under the Flushability Test at least 95% of the time in one flush.
6. The individual package of Claim 1 wherein the time required for said wrapper to disperse into at least two fragments as measured by the Water Dispersion Test is less than two hours.
- 30 7. The individual package of Claim 1 wherein said wrapper causes drain blockage of less than 80%.



8. The individually packaged absorbent interlabial device wherein said absorbent interlabial device comprises:

a central absorbent portion comprising a longitudinal dimension, a width, a height, wherein said longitudinal dimension is greater than said height, an upper portion, and a lower portion thereof, said upper portion facing toward the vestibule floor of said wearer during insertion into said interlabial space and leading said lower portion during insertion therein, said upper portion having a longitudinal axis, said lower portion being opposed to said upper portion and upon insertion of said absorbent device into said interlabial space said lower portion facing away from the floor of the vestibule of said wearer; and

an individual package for said absorbent interlabial device comprising a flexible sheet which is folded about said absorbent interlabial device relative to said longitudinal axis of said lower portion forming a longitudinal fold, longitudinal edges, and transverse side edges wherein said longitudinal edges and said transverse side edges are sealed forming said individual package, which when said individual package is opened, provides the user with a sanitary wiping device to wipe the labia while inserting said absorbent interlabial device into the interlabial space.

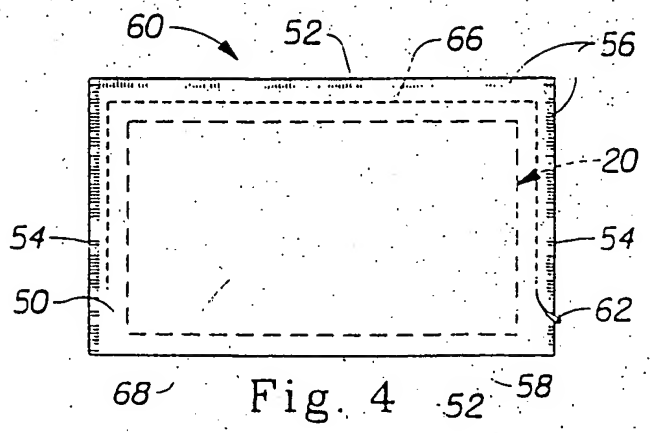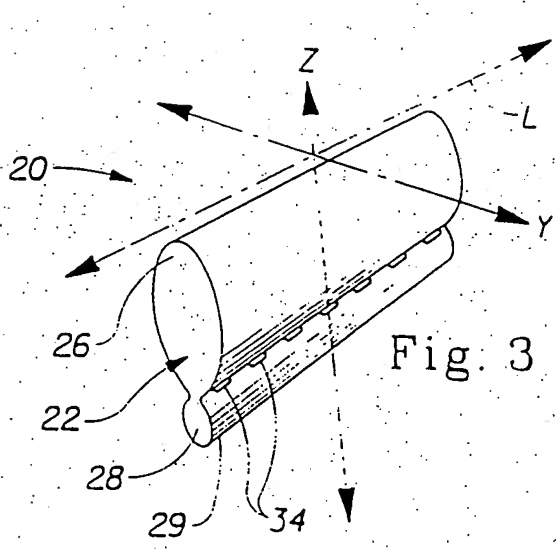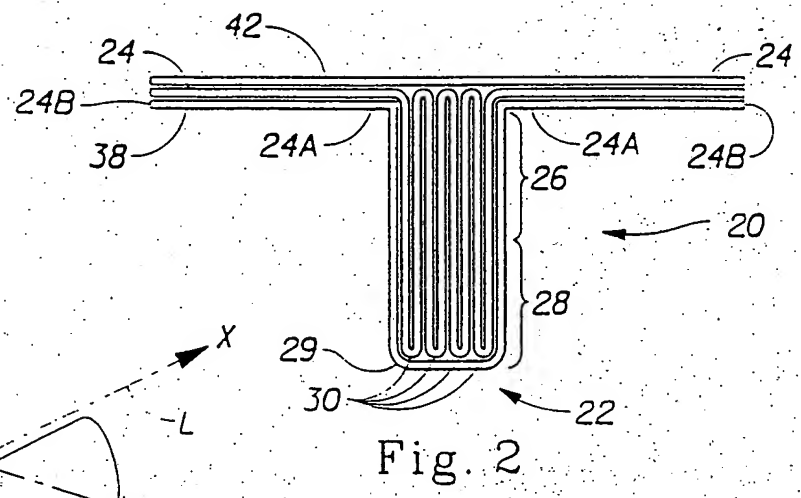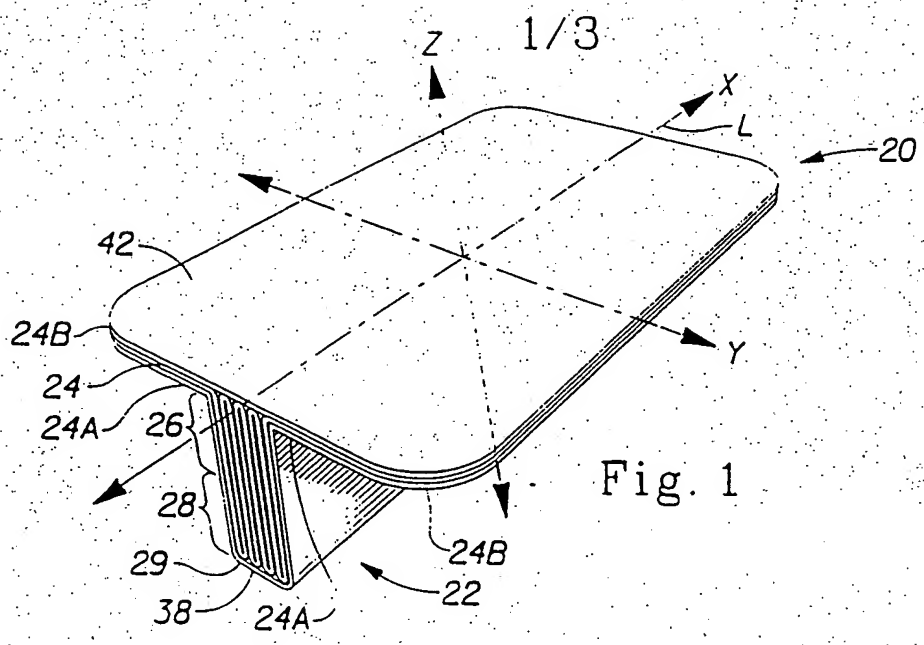

2/3

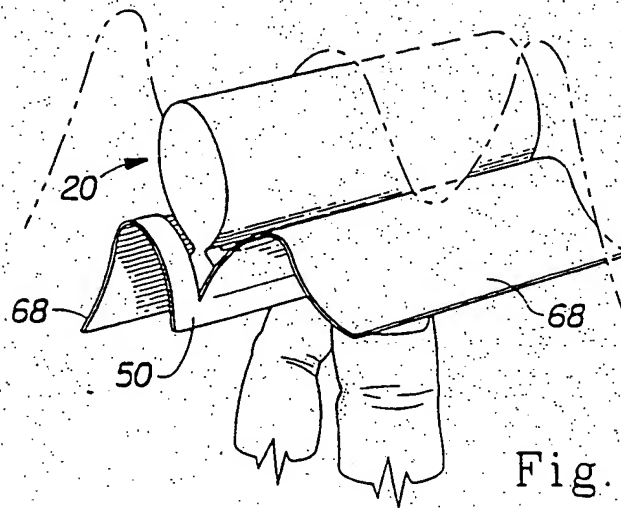


Fig. 5

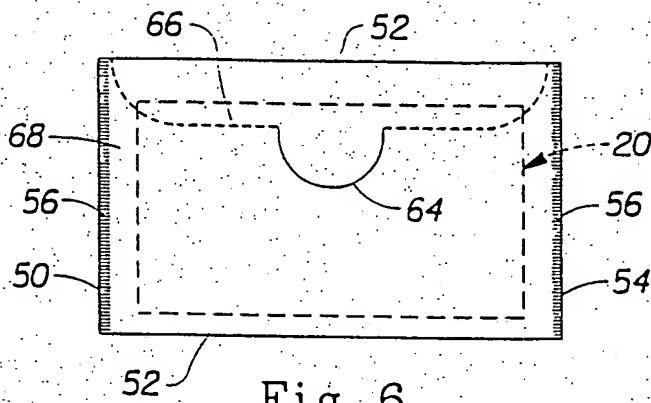


Fig. 6

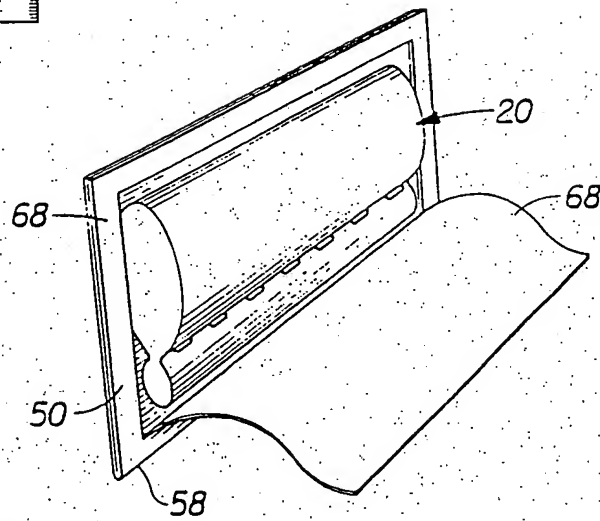


Fig. 8

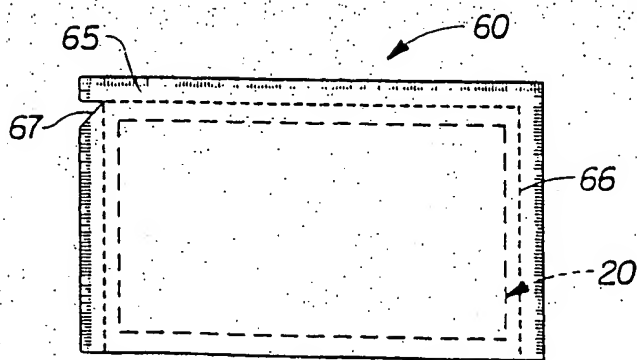


Fig. 7

3/3

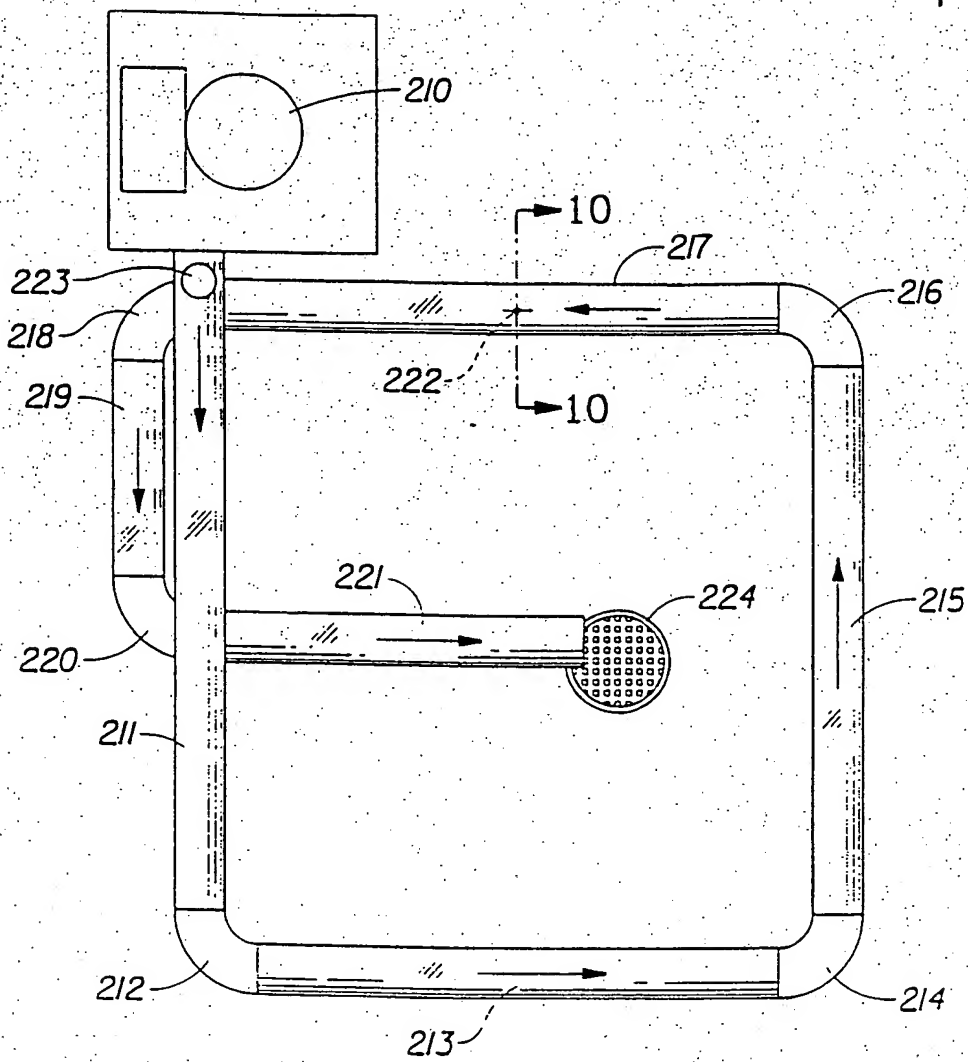


Fig. 9

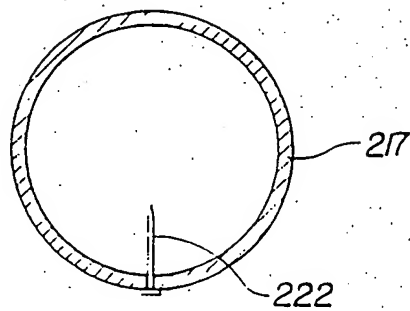


Fig. 10